



Receiver REC 300 Digital

en Operating instructions


Operating instructions

The STABILA REC 300 Digital is a simple-to-use receiver for the rapid capture of rotating lasers. The REC 300 Digital receiver can receive laser beams from rotation lasers, even when these are invisible to the naked eye.

The distance to the “on line” position is indicated digitally.

We have endeavoured to explain the unit's handling and functioning in as clear and comprehensible manner as possible. If, however, you still have any unanswered questions, we should be pleased to provide advice over the telephone at any time on the following telephone number: +49 / 6346 / 309-0

Main components

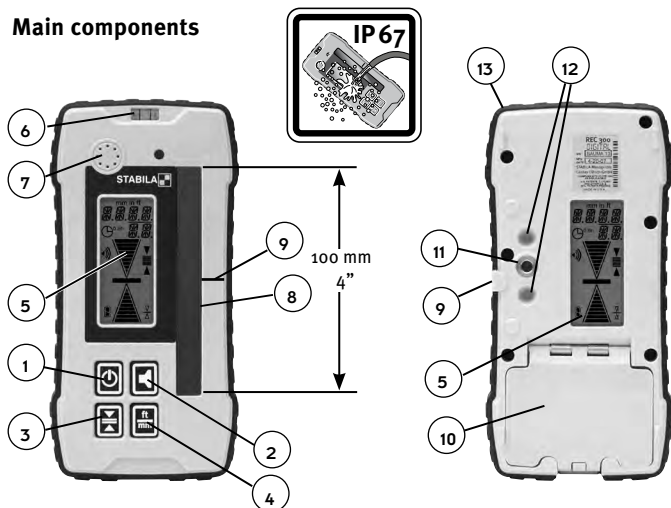

1. ON/OFF button
2. Volume button
3. Accuracy button
4. Measuring unit button
5. LCD
6. Vial
7. Beeper

8. Laser receiver glass 100 mm / 4"
9. "In line" marks
10. Battery compartment cover
11. Fixing thread for the clamp
12. Clamp Guides
13. Shock protection

Getting started


Press the ON/OFF button (1). An audio signal and a short flash from the display will confirm, that the instrument is switched on. The instrument will now calibrate itself.



Press the ON/OFF button (1) quickly once (2sec) to switch the instrument off. If the instrument is not used, it will automatically switch itself off after 30 minutes.

Height difference display: analogue

20 display steps indicate the divergence from the centre of the laser line. The central bar indicates the "in line" position of the REC 300 Digital. The arrow increases in size as the distance from the "in line" position increases.

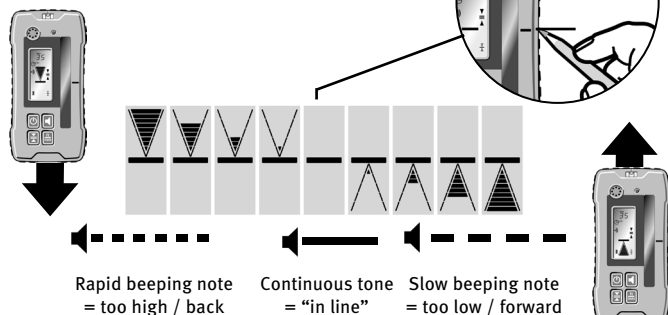

Audio signals


Setting the volume

The volume is increased/decreased by repeatedly pressing the button (2): Loud (a), soft (b) or off.

- 2 If the instrument is set to "silent" only a short beep is emitted when the laser beam is received.



Height difference display: digital

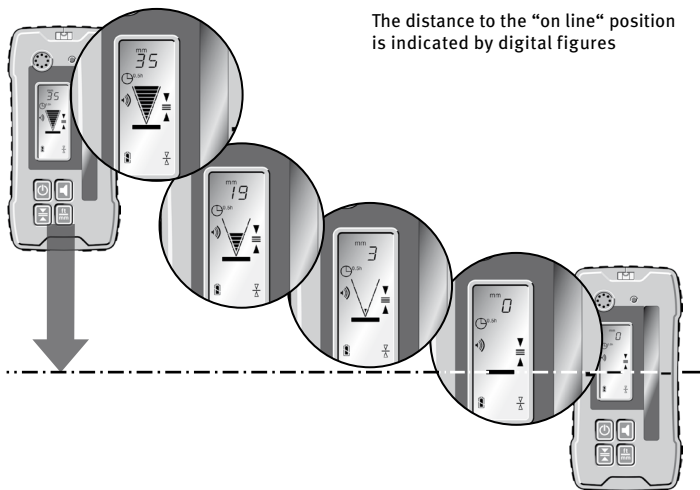

The distance to the “on line” position is indicated by digital figures

Measuring modes

Setting the accuracy level



The icons appear permanently



Fine

± 1,0 mm
± 0,05 in
± 1/16 in
± 0,005 ft



Coarse

± 5,0 mm
± 0,2 in
± 1/4 in
± 0,02 ft

The display appears only briefly

~ 1 sec

The setting selected remains in memory after the unit is switched off.

Setting the measuring unit



The display appears only briefly ~ 1 sec



The setting selected remains in memory after the unit is switched off.

Replacing the batteries

LCD



Full:
Batteries
OK



Half:
Initial
Warning



Empty:
Approximately
30 Minutes
Remaining




Flashing:
Change
Batteries!

Slide the battery cover (10) in the direction of the arrow and insert new batteries in accordance with the symbols in the battery compartment.

2 x 1,5V

Mignon cells Alkaline,
Size AA, LR6

Mignon
AA
LR6

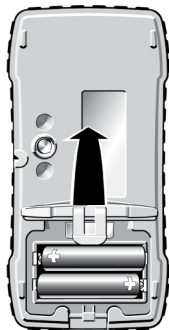


Remove the batteries if the unit will not be used for a long period !



Battery compartment cover. Water-tight. Protection against water and dust is ensured by the pressure of the cover against the seal. IP 67.

Bracket

1. Securing screw - for securing to the rear side of the receiver.
2. Guide cones - assist in quickly and securely fixing the bracket to the receiver.
3. Reading reference
4. Securing knob. Turning the securing knob fixes / releases the clamp with the receiver to/from the levelling staff.
5. Moveable clamping jaw - for fixing to the levelling staff.

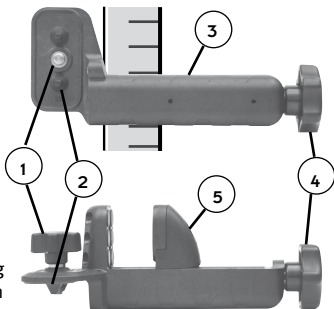

Care and maintenance

Cleaning: Please do not remove dust and dirt from the receiving or display window by using dry cloths or abrasive materials as this procedure scratches the windows.

A soft cloth and mild soap and water are effective.

The unit may be submerged under water or sprayed with a low pressure hose if necessary. Do not use any other fluids other than water or glass- cleaner, as they may attack polymer components.

Prohibited Uses

- Operation without instruction.
- Operation other than the intended uses.
- Opening the detector, except the battery compartment.
- Modification or conversion of the detector.




Important information

- The person in charge of the detector must understand the instructions in this manual and ensure other users do also.
- Periodically carry out test measurements, particularly after the detector has been subjected to abnormal use and before and after important measurements.

Positioning and adjustment of the instrument.

When setting up the instrument, take care that the laser beam does not produce any unwanted reflections from reflective surfaces.

These reflections may also be captured by the receiver and produce incorrect readings.



Recycling programme for our EU customers:

In accordance with the WEEE regulations, STABILA provides a disposal programme for electronic products at the end of their service life. For more details, please contact: +49 / 6346 / 309-0



Technical data

Accuracy	Fine:	± 1,0 mm	0,05 in	1/16 in	0,5/100 ft
	Coarse:	± 5,0 mm	0,20 in	1/4 in	2,0/100 ft
Detectable Spectrum:		610 nm - 780 nm			
Beeper Volumes:		Loud: ~ 105 dBA		Low: ~ 85 dBA	
Batteries:		2 x 1,5V Mignon cells Alkaline , Size AA,LR 6			
Operating life:		70 hours			
Automatic Shut Off:		30 minutes			
Operating temperature range:		-20°C to +60°C			
Storage temperature range:		-40°C to +70°C			

Subject to technical modifications.

Guarantee terms and conditions

In addition to the statutory rights to which the purchaser is entitled and which are not limited by this guarantee, STABILA guarantees the instrument against defects and the absence of the warranted characteristics resulting from material or manufacturing defects for a period 24 months from the date of purchase. This guarantee is valid worldwide. STABILA has the right to decide at its own discretion whether the defects will be rectified by being repaired or whether the instrument will be replaced. STABILA accepts no further liability. Defects caused by improper handling (e.g. damage caused by the effects of powerful electric currents, operating the instrument with the incorrect voltage / type of current, use of unsuitable power sources) as well as modifications to the instrument undertaken by the purchaser or third parties invalidate the guarantee. No liability is accepted for normal wear and tear and minor defects which do not detract from the function of the instrument. Please send your claims under the guarantee along with the completed guarantee certificate to the guarantor (See last page):



STABILA Messgeräte
Gustav Ullrich GmbH

P.O. Box 13 40 / D-76851 Annweiler
Landauer Str. 45 / D-76855 Annweiler

Tel.: + 49 (63 46 / 309 - 0
Fax: +49 (63 46 / 309 - 480

e-mail: info@stabila.de
www.stabila.com

USA
Canada

STABILA Inc.
332 Industrial Drive
South Elgin, IL 60177
1.800.869.7460
www.stabila.com