

VOLTCRAFT®

**DSO-111 Oscilloscope
User Manual**

Table of Contents

1. General Safety Requirements.....	1
2. Safety Terms and Symbols.....	2
3. User Guidebook.....	4
Structure of the Oscilloscope.....	4
Front Panel.....	4
Rear Panel.....	6
General Inspection.....	7
Basic Operation.....	7
Probe Compensation.....	8
Set the Probe Attenuation Coefficient.....	9
Use the Probe Safely.....	9
X-Y Mode.....	10
4. Troubleshooting.....	12
5. Technical Specifications.....	13
General Technical Specifications.....	14
6. Appendix.....	15
Appendix A: Enclosure.....	15
Appendix B: General Care and Cleaning.....	15

1. General Safety Requirements

Before use, please read the following safety precautions to avoid any possible bodily injury and to prevent this product or any other connected products from damage. To avoid any contingent danger, ensure this product is only used within the range specified.

Only the qualified technicians can implement the maintenance.

To avoid Fire or Personal Injury:

- **Connect the probe correctly.** The grounding end of the probe corresponds to the grounding phase. Please don't connect the grounding end to the positive phase.
- **Use Proper Power Cord.** Use only the power cord supplied with the product and certified to use in your country.
- **Connect or Disconnect Correctly.** When the probe or test lead is connected to a voltage source, please do not connect and disconnect the probe or test lead at random.
- **Product Grounded.** This instrument is grounded through the power cord grounding conductor. To avoid electric shock, the grounding conductor must be grounded. The product must be grounded properly before any connection with its input or output terminal.

When powered by AC power, it is not allowed to measure AC power source directly, because the testing ground and power cord ground conductor are connected together, otherwise, it will cause short circuit.

- **Check all Terminal Ratings.** To avoid fire or shock hazard, check all ratings and markers of this product. Refer to the user's manual for more information about ratings before connecting to the instrument.
- **Do not operate without covers.** Do not operate the instrument with covers or panels removed.
- **Use Proper Fuse.** Use only the specified type and rating fuse for this instrument.
- **Avoid exposed circuit.** Do not touch exposed junctions and components when the instrument is powered.
- **Do not operate if in any doubt.** If you suspect damage occurs to the instrument, have it inspected by qualified service personnel before further operations.
- **Use your Oscilloscope in a well-ventilated area.** Make sure the instrument installed with proper ventilation, refer to the user manual for more details.
- **Do not operate in wet conditions.**
- **Do not operate in an explosive atmosphere.**
- **Keep product surfaces clean and dry.**

2. Safety Terms and Symbols

Safety Terms

Terms in this manual. The following terms may appear in this manual:



Warning: Warning indicates the conditions or practices that could result in injury or loss of life.



Caution: Caution indicates the conditions or practices that could result in damage to this product or other property.

Terms on the product. The following terms may appear on this product:

Danger: It indicates an injury or hazard may immediately happen.

Warning: It indicates an injury or hazard may be accessible potentially.

Caution: It indicates a potential damage to the instrument or other property might occur.

Safety Symbols

Symbols on the product. The following symbol may appear on the product:



Hazardous Voltage



Refer to Manual



Protective Earth Terminal



Chassis Ground



Test Ground


2.Safety Terms and Symbols

To avoid body damage and prevent product and connected equipment damage, carefully read the following safety information before using the test tool. This product can only be used in the specified applications.

Warning:

In X-Y mode, the X Input and Y Input of the oscilloscope are not electrically isolated. The channels should adopt a common ground during measuring. To prevent short circuits, the 2 probe grounds must not be connected to 2 different non-isolated DC levels.

The diagram of the oscilloscope ground wire connection:

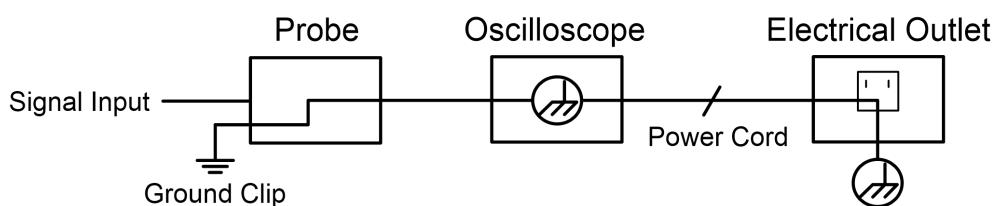

Warning:

To avoid fire or electrical shock, when the oscilloscope input signal connected is more than 42V peak (30Vrms) or on circuits of more than 4800VA, please take note of below items:

- Only use accessory insulated voltage probes and test lead.
- Check the accessories such as probe before use and replace it if there are any damages.
- Remove probes, test leads and other accessories immediately after use.
- Do not apply input voltages above the rating of the instrument because the probe tip voltage will directly transmit to the oscilloscope. Use with caution when the probe is set as 1:1.
- Do not use exposed metal BNC or banana plug connectors.
- Do not insert metal objects into connectors.

3. User Guidebook

Structure of the Oscilloscope

This chapter makes a simple description of the operation and function of the front panel of the oscilloscope, enabling you to be familiar with the use of the oscilloscope in the shortest time.

Front Panel

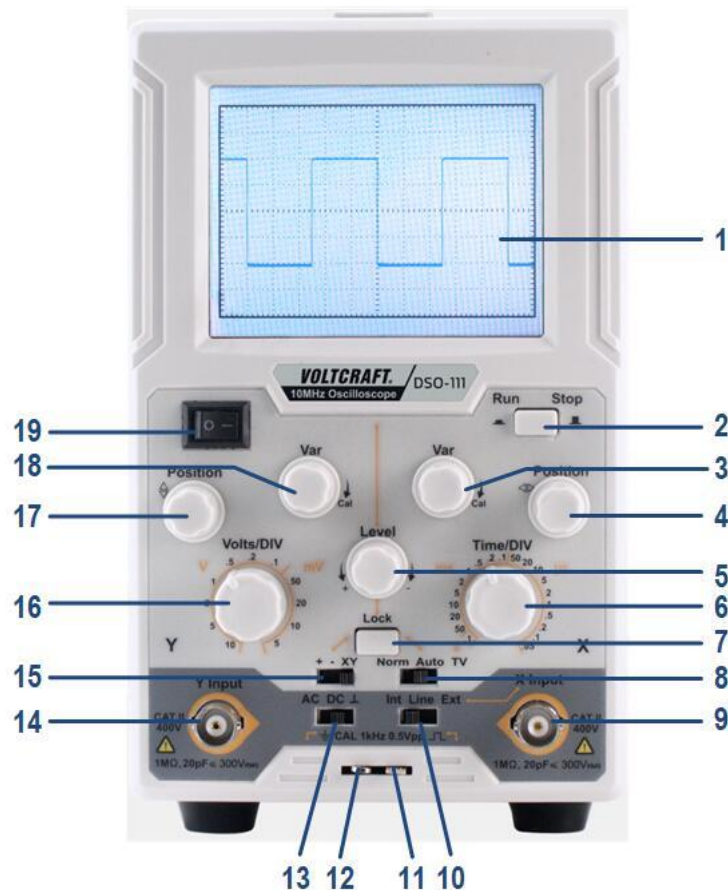


Figure 3- 1 Front panel

No.	Name	Description
1	Display screen	Display the trace.
2	Run/Stop	Enable or disable sampling on input signals.
3	Var (right side)	Provides continuously variable sweep rate. Turn clockwise until the waveform does not change is the calibration position.
4	◀▷Position	Horizontal positioning control of trace on the screen.

3. User Guidebook

5	Level	Control signal trigger to sweep at certain level. Towards "-": The triggering level moves downward on the display waveform. Towards "+": The triggering level moves upward on the display waveform.
6	Time/DIV	Select the sweep rate.
7	Lock	When the Lock button is pressed down, the triggering level is automatically maintained at optimum value irrespective of the signal amplitude, requiring no manual adjustment of triggering level.
8	Norm/Auto/TV	Select the desired trigger mode. Norm: No trace on screen if no signal. Trace is only generated when adequate trigger signal is present. Auto: a single trace shown on screen even no signal. Automatically reverts to triggered sweep operation when adequate triggered signal is present. Needs to adjust the Level. TV: Used to show TV signals.
9	X Input	When switching to XY mode, it's X input terminal. When switching the trigger source to Ext, it's external trigger input terminal.
10	Int/Line/Ext	Switch to select the Trigger Source. Int: Select internal signal as trigger source signal. Line: Select AC power line as trigger signal. Ext: The external signal applied through X Input terminal is used for the external triggering source signal.
11	CAL signal	Provide calibration square wave for 0.5Vpp range, frequency=1kHz. Used for adjusting probe compensation and adjusting the vertical & horizontal sensitivity.
12	CAL ground	Ground wire connector of the calibration signal.
13	AC/DC/⊥	Switch for selecting coupling mode. AC: Block the DC component of the input signal. DC: Pass both AC and DC components of the input signal. ⊥ (GND): Disconnect the input signal.
14	Y Input	Vertical input terminal.

3.User Guidebook

15	+/-/XY	<p>+: Trigger on rising slope. Triggering occurs when the triggering signal crosses the triggering level in positive-going direction.</p> <p>-: Trigger on falling slope. Triggering occurs when the triggering signal crosses the triggering level in negative-going direction.</p> <p>XY: This position is used when using the instrument as an X-Y oscilloscope.</p>
16	Volts/DIV	Adjusting sensitivity of vertical system.
17	◊Position	Control vertical position of trace on the screen.
18	Var (left side)	Continuously adjusting the sensitivity of vertical system. Turn clockwise until the waveform does not change is the calibration position.
19	Power switch	Main power on/off.

Rear Panel

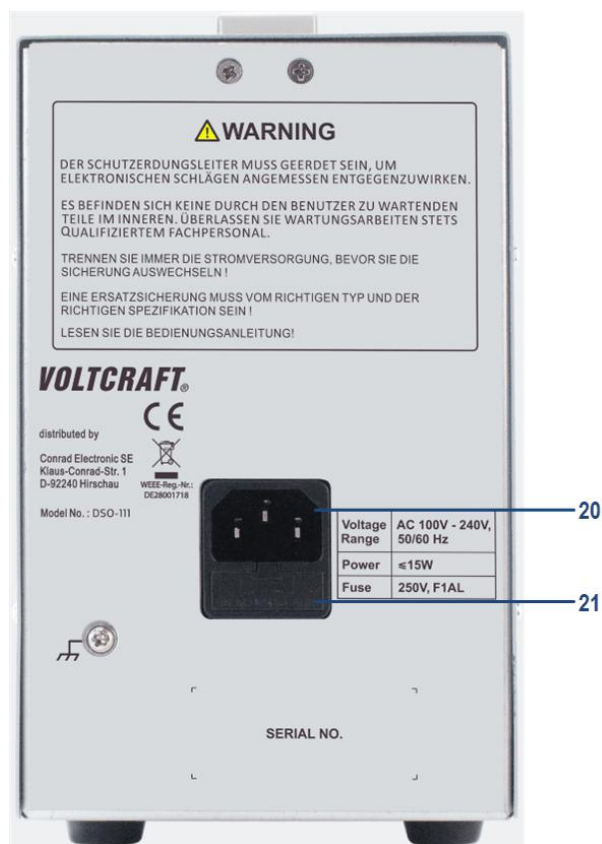


Figure 3-2 Rear Panel

No.	Name	Description
20	AC Power input connector	Connect the supplied AC power cord to this connector.
21	Fuse holder	Fuse rating is 1A, T class, 250 V.

General Inspection

After you get a new oscilloscope, it is recommended that you should make a check on the instrument according to the following steps:

1. Check whether there is any damage caused by transportation.

If it is found that the packaging carton or the foamed plastic protection cushion has suffered serious damage, do not throw it away first till the complete device and its accessories succeed in the electrical and mechanical property tests.

2. Check the Accessories

The supplied accessories have been already described in the "Appendix A: Enclosure" of this manual. You can check whether there is any loss of accessories with reference to this description. If it is found that there is any accessory lost or damaged, please get in touch with the distributor of our responsible for this service or our local offices.

3. Check the Complete Instrument

If it is found that there is damage to the appearance of the instrument, or the instrument cannot work normally, or fails in the performance test, please get in touch with our distributor responsible for this business or our local offices. If there is damage to the instrument caused by the transportation, please keep the package. With the transportation department or our distributor responsible for this business informed about it, a repairing or replacement of the instrument will be arranged by the us.

Basic Operation





- Set the switches and controls on the front panel as shown below.

Position for control switches

Item	No. in Figure 3-1 Front panel	Setting
Power switch	19	○ pressed down
Volts/DIV	16	0.1 V
Norm/Auto/TV	8	Auto
Time/DIV	6	0.5 ms
+/-/XY	15	+

3. User Guidebook


Int/Line/Ext	10	Int
AC/DC/⊥	13	⊥
Lock	7	Pressed down

2. Connect the power cord to the AC line outlet. Press the power switch  on the front panel to power on, the screen will light up. A few seconds later, a trace will appear on the screen.
3. Align the trace with the horizontal center line of the graticule by adjusting the  Position knob.
4. Connect the probe to the Y Input terminal and apply the 0.5 V_{pp} CALIBRATOR signal to be probe tip.
5. Set the AC/DC/⊥ switch to the AC state. A square waveform will be displayed on the screen.
6. For signal viewing, set the Volts/DIV switch and Time/DIV switch in appropriate positions so that signal waveform is displayed clearly.
7. Adjust the  Position and  Position controls in appropriate positions so that the displayed waveform is aligned with the graticule and voltage and period can be read conveniently.

Probe Compensation

When connect the probe with the input channel for the first time, make this adjustment to match the probe with the input channel. The probe which is not compensated or presents a compensation deviation will result in the measuring error or mistake. For adjusting the probe compensation, please carry out the following steps:

1. Set the switch in the probe to 10X. (see "*Set the Probe Attenuation Coefficient*" on P9).
2. Connect the probe BNC connector to the Y Input terminal. Connect the probe tip to the calibration signal on the front panel (see 11 of Figure 3- 1 Front panel). Connect the reference wire clamp to the ground wire connector of the calibration signal (see 12 of Figure 3- 1 Front panel).
3. Check the displayed waveforms and regulate the probe till a correct compensation is achieved (see *Figure 3- 3* and *Figure 3- 4*).

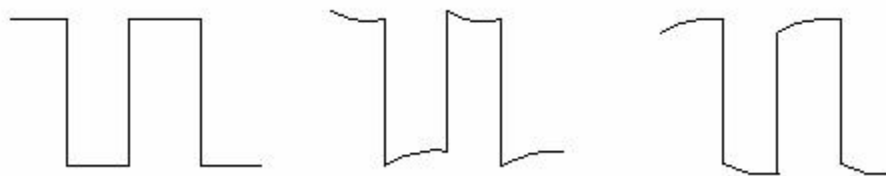

Compensated correctly Overcompensated Under compensated

Figure 3-3 Displayed Waveforms of the Probe Compensation

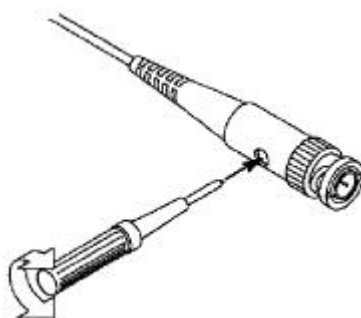


Figure 3-4 Adjust Probe

Set the Probe Attenuation Coefficient

The probe has several attenuation coefficients, which will influence the vertical scale factor of the oscilloscope.

The set values of the probe switch are 1X and 10X (see *Figure 3-5*).

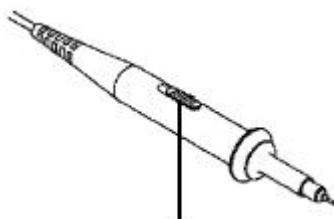


Figure 3-5 Attenuation Switch



Caution:

When the attenuation switch is set to 1X, the probe will limit the bandwidth of the oscilloscope in 5MHz or 6MHz. To use the full bandwidth of the oscilloscope, the switch must be set to 10X.

Use the Probe Safely

The safety guard ring around the probe body protects your finger against any electric shock, shown as *Figure 3-6*.



Figure 3-6 Finger Guard



Warning:

To avoid electric shock, always keep your finger behind the safety guard ring of the probe during the operation.

To protect you from suffering from the electric shock, do not touch any metal part of the probe tip when it is connected to the power supply.

Before making any measurements, always connect the probe to the instrument and connect the ground terminal to the earth.

X-Y Mode

Examine the Phase Difference between Signals of two Channels

X-Y mode is a very useful when examining the Phase difference of two signals.

1. Set the +/-XY control on the front panel to the **XY** position.
2. Set the switch in the probe to 1X or 10X, depend on your need (see "*Set the Probe Attenuation Coefficient*" on P9).
3. Connect the probe of Y Input to the Y-axis signal (vertical axis signal). Connect the probe of X Input to the X-axis signal (horizontal axis signal).
4. Turn the **Volts/DIV** knob to set the vertical scale of Y-axis signal. The vertical scale of X-axis signal is fixed as 0.5V/DIV.
5. The vertical position is adjusted using the ∇ **Position** knob. The horizontal position is adjusted using the $\triangleleft \triangleright$ **Position** knob.
6. With the elliptical oscillogram method adopted, observe and calculate the phase difference (see *Figure 3-7*).

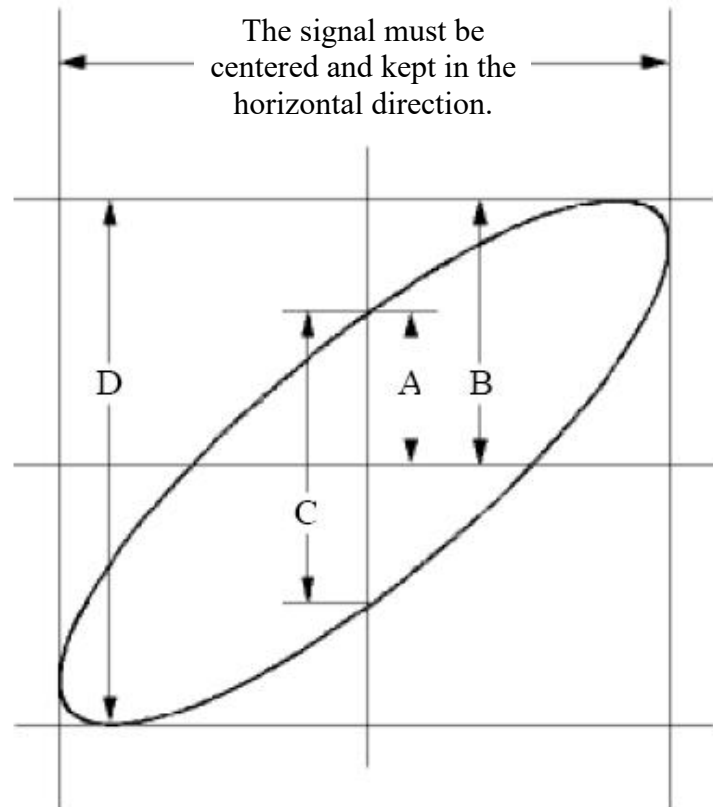


Figure 3-7 Lissajous Graph

Based on the expression $\sin(\theta) = A/B$ or C/D , thereinto, θ is the phase difference angle, and the definitions of A, B, C, and D are shown as the graph above. As a result, the phase difference angle can be obtained, namely, $\theta = \pm \arcsin(A/B)$ or $\pm \arcsin(C/D)$. If the principal axis of the ellipse is in the I and III quadrants, the determined phase difference angle should be in the I and IV quadrants, that is, in the range of $(0 - \pi/2)$ or $(3\pi/2 - 2\pi)$. If the principal axis of the ellipse is in the II and IV quadrants, the determined phase difference angle is in the II and III quadrants, that is, within the range of $(\pi/2 - \pi)$ or $(\pi - 3\pi/2)$.

4. Troubleshooting

1. Oscilloscope is powered on but no display.

- Check whether the power connection is connected properly.
- Check whether the fuse which is beside the AC power input jack is blew (the cover can be pried open with a straight screwdriver).
- Restart the instrument after completing the checks above.
- If the problem persists, please contact us and we will be under your service.

2. After acquiring the signal, the waveform of the signal is not displayed in the screen.

- Check whether the probe is properly connected to the signal connecting wire.
- Check whether the signal connecting wire is correctly connected to the BNC (namely, the channel connector).
- Check whether the probe is properly connected with the object to be measured.
- Check whether there is any signal generated from the object to be measured (the trouble can be shot by the connection of the channel from which there is a signal generated with the channel in fault).
- Make the signal acquisition operation again.

3. The measured voltage amplitude value is 10 times or 1/10 of the actual value.

Look at the attenuation ration of the probe (see "*Set the Probe Attenuation Coefficient*" on P9).

4. There is a waveform displayed, but it is not stable.

- Check whether the trigger source (**Int/Line/Ext** controls on the front panel) is in conformity with the signal channel used in the practical application.
- Press down the **Lock** button on the front panel.

5. Technical Specifications

Unless otherwise specified, the technical specifications applied are for the oscilloscope only, and probes attenuation set as 10X. Only if the oscilloscope fulfills the following condition at first, these specification standards can be reached.

- This instrument should run for at least 30 minutes continuously under the specified operating temperature.

All specification standards can be fulfilled, except one(s) marked with the word "Typical".

Performance Characteristics		Instruction
Bandwidth	DC	0 – 10 MHz
	AC	10 Hz – 10 MHz
Channel Q'nty		1
Acquisition	Run/Stop	supported
	Sampling Rate	100M Sa/s
Input	Input Coupling	DC, AC, and ground
	Input Impedance	1 MΩ ± 2%, in parallel with 20 pF±5 pF
	Max. Input Voltage	400V (DC+AC, PK - PK)
Horizontal System	Sampling Rate Range	0.5 Sa/s - 100 MSa/s
	Interpolation	sin(x)/x
	Scanning Speed (s/DIV)	0.05μs/DIV - 0.1s/DIV, step by 1 - 2 - 5
	Sampling Rate / Relay Time Accuracy	±100 ppm
	Trimming Ratio	≥ 2.5:1
Vertical system	Sensitivity	5 mV/DIV - 10 V/DIV
	Displacement	±10 DIV
	Analog Bandwidth	10 MHz
	Low Frequency	≥ 10 Hz (at input, AC coupling, -3 dB)
	Rise Time (at input, typical)	≤ 30 ns
	Trimming Ratio	≥ 2.5:1

X-Y Mode

Sensitivity	X: 0.5V/DIV, Y: 0.1V/DIV - 1V/DIV
Bandwidth (-3dB)	DC: 0 - 1MHz, AC: 10Hz - 1MHz

Trigger

Trigger Level Range	Internal	±4 DIV from the screen center
Trigger Level Accuracy (typical)	Internal, External	±0.3 DIV
Trigger Lock		supported
Edge Trigger	Slope	rising, falling

5. Technical Specifications

Video Trigger	Modulation	supported standard: NTSC, PAL and SECAM broadcast systems
Ext. Trigger Input Impedance		1 M Ω \pm 2%, in parallel with 20 pF \pm 5 pF
Ext. Trigger Max. Input Voltage		400 Vpp
Trigger Source		Int, Line, Ext
Trigger Mode		Norm, Auto, and TV
Output of the Probe Compensator		
Output Voltage (typical)		square, 0.5 Vpp \pm 2%
Frequency (typical)		square wave of 1 kHz (\pm 1%)

General Technical Specifications

Display

Display Type	3.7" LCD, TFT screen
Display Resolution	320 (horizontal) x 240 (vertical) pixels
Display Color	65536 colors
Power	
Mains Voltage	100 - 240 VACRMS, 50/60 Hz, CAT II
Power Consumption	< 15 W
Fuse	1A, T class, 250 V
Environment	
Temperature	working temperature: (0 °C) - (+40 °C)
	storage: (-20 °C) - (+60 °C)
Relative Humidity	\leq 90%
Height	operating: 3,000 m
	non-operating: 15,000 m
Cooling Method	natural cooling
Mechanical Specifications	
Dimension (D/H/W)	288 mm x 195 mm x 117 mm
Weight	Approx. 1.8 kg

Interval Period of Adjustment:

One year is recommended for the calibration interval period.

6. Appendix

Appendix A: Enclosure

(The accessories subject to final delivery.)

Standard Accessories:

Power cord x 1

Quick guide EN x 1

Quick guide DE x 1

Safety Hintsheet x 1

Probe x 1

Probe adjust x 1

Fuse x 1

Appendix B: General Care and Cleaning

General Care

Do not store or leave the instrument where the display will be exposed to direct sunlight for long periods of time.

Caution: To avoid any damage to the instrument or probe, do not exposed it to any sprays, liquids, or solvents.

Cleaning

Inspect the instrument and probes as often as operating conditions require.

To clean the instrument exterior, perform the following steps:

1. Wipe the dust from the instrument and probe surface with a soft cloth. Do not make any scuffing on the transparent LCD protection screen when clean the LCD screen.
2. Disconnect power before cleaning your Oscilloscope. Clean the instrument with a wet soft cloth not dripping water. It is recommended to scrub with soft detergent or fresh water. To avoid damage to the instrument or probe, do not use any corrosive chemical cleaning agent.



Warning: Before power on again for operation, it is required to confirm that the instrument has already been dried completely, avoiding any electrical short circuit or bodily injury resulting from the moisture.
