

Dasqua®


PRODUCT INSTRUCTION

ZERO SETTING DEVICE


Please read the product instruction carefully and use the product correctly under the instruction

Structure

Type 1

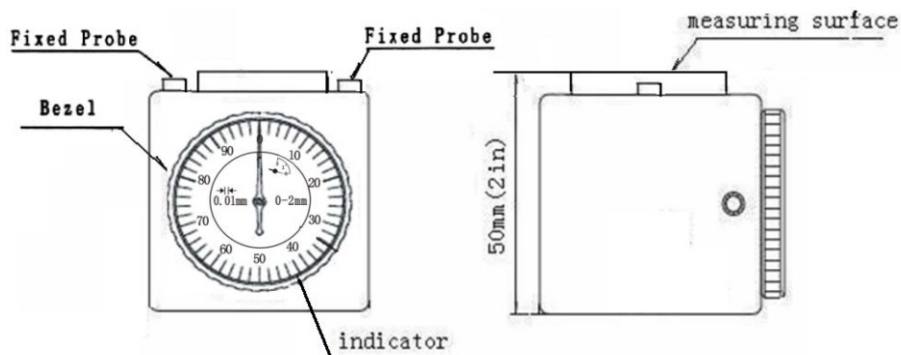

Type 2

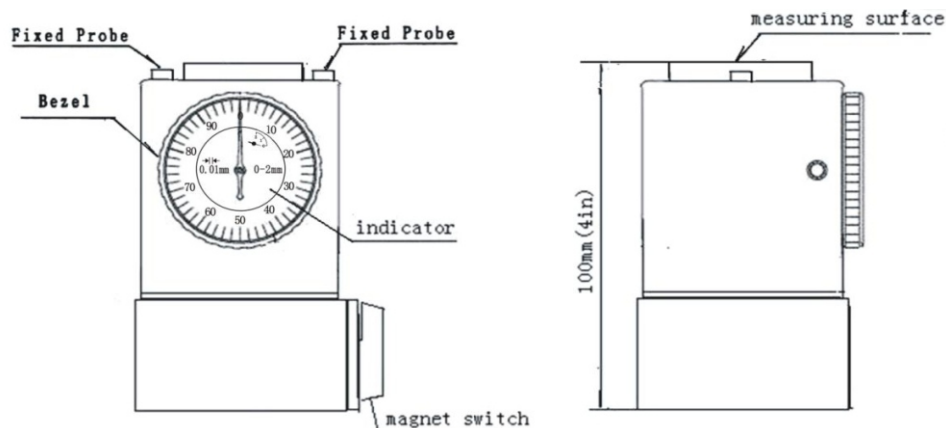

Features

- a. Type I : Height 50mm (2in); Type II : Height 100mm (4in)
- b. Measuring range: 2 mm (0.1in), Indicator graduation: 0.01mm (0.001in or 0.0005in)
- c. The two Fixed Probes are used as the calibration height of the product.

PRODUCT INSTRUCTION

Dasqua®

Usage

- a. Use the “Zero” level straight edge pressing down the measuring surface and the Fixed Probe at the same level.
- b. Put on the work piece, cutter touch probe side, if gauge is Type II, rotate the magnet switch to “ON” . When the long-needle and short-needle moving to "0" at the same time, the distance of the cutter with work piece is 50mm for Metric Type I (2in inch for Type I) or 100mm for metric type II (4in for inch Type II).

Notice

- a. To make sure the accuracy of the product,you should avoid putting it on the unprocessed Gross-pui surface.
- b. Please use the middle area of the measuring surface as possible as you can.
- c. To avoid demagnetization, please not approach to the heat source more than 100 degrees Celsius when you use the magnetic product,with magnetization on the bottom.
- d. Please make sure to keep the measuring surface and the bottom clean, affix the anti-rust paper to both of them to avoid rust when not use.
- e. The product should be used 1hour later,when the indoor temperature reaches 18°C to 22°C .


Dasqua® NULLSTELLVORRICHTUNG

PRODUKTANLEITUNG


Bitte lesen Sie die Produktanleitung sorgfältig durch und verwenden Sie das Produkt entsprechend der Anleitung.

Struktur

Typ I

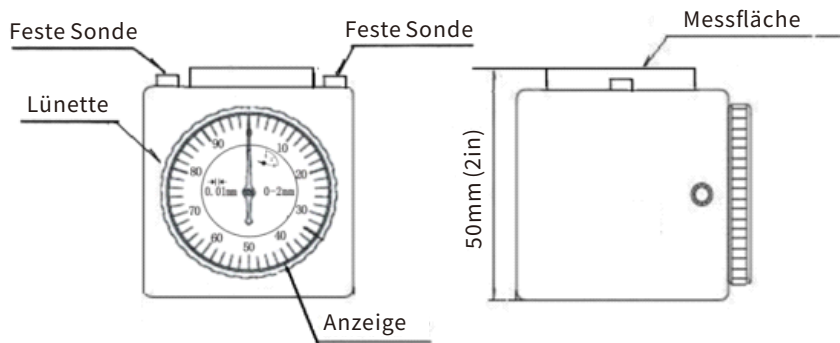

Typ II

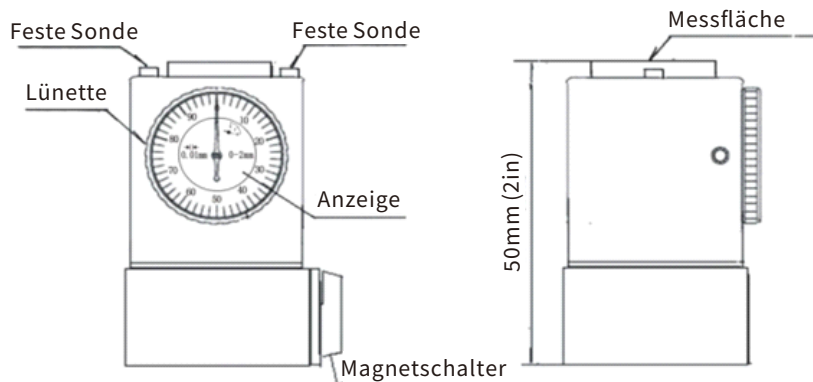

PRODUKTANLEITUNG

Dasqua®

Merkmale

- a. Typ I: Höhe 50mm (2in); Typ II: Höhe 100mm (4in)
- b. Messbereich: 2 mm (0,1in), Anzeigeskala: 0,01mm (0,001in oder 0,0005in)
- c. Die beiden festen Sonden werden als Kalibrierungshöhe des Produkts verwendet.

Verwendung

- a. Verwenden Sie die "Null" Ebene gerader Kante, indem Sie die Messfläche und die feste Sonde auf demselben Niveau nach unten drücken.
- b. Setzen Sie das Werkstück auf, der Messer berührt die Sondenseite. Wenn das Messgerät vom Typ II ist, drehen Sie den Magnetschalter auf "ON". Wenn sich die lange und die kurze Nadel gleichzeitig auf "0" bewegen, beträgt der Abstand des Messers zum Werkstück 50mm für den metrischen Typ I (2 Zoll für Typ I) oder 100mm für den metrischen Typ II (4 Zoll für Typ II).

Hinweis

- a. Um die Genauigkeit des Produktes zu gewährleisten, sollten Sie es nicht auf die unbearbeitete Gross-Pui Oberfläche legen.
- b. Bitte verwenden Sie möglichst den mittleren Bereich der Messfläche.
- c. Um eine Entmagnetisierung zu vermeiden, nähern Sie sich bitte nicht der Wärmequelle von mehr als 100 Grad Celsius, wenn Sie das magnetische Produkt verwenden, mit Magnetisierung auf der Unterseite.
- d. Bitte achten Sie darauf, die Messfläche und die Unterseite sauber zu halten, kleben Sie das Anti-Rost-Papier auf beide, um Rost zu vermeiden, wenn Sie es nicht benutzen.
- e. Das Gerät sollte erst nach 1 Stunde benutzt werden, wenn die Raumtemperatur 18°C bis 22°C erreicht hat.