

User instructions

Metallurgical inverted microscope

KERN OLM 170

OLM 170

Version 1.0
01/2023





KERN OLM 170

Version 1.0 01/2023

User instructions

Metallurgical inverted microscope

Table of contents

1	Before use	3
1.1	General notes.....	3
1.2	Notes on the electrical system.....	3
1.3	Storage	4
1.4	Maintenance and cleaning.....	5
2	Nomenclature	6
3	Technical data / Features	8
4	Assembly	10
4.1	Reflected light unit	11
4.2	Objectives	13
4.3	Eyepieces	14
4.4	Specimen stage	14
5	Operation	15
5.1	Getting started	15
5.2	(Pre-) focussing	16
5.3	Adjusting the interpupillary distance	17
5.4	Diopter adjustment.....	17
5.5	Adjusting the magnification	18
5.6	Using eye cups	19
5.7	Adjusting the illumination	20
6	Changing the bulb	21
7	Using optional accessories.....	22
7.1	Camera connection	22
8	Trouble shooting.....	23
9	Service	25
10	Disposal.....	25
11	Further information.....	25

1 Before use

1.1 General notes

You must open the packaging carefully, to make sure that none of the accessories in the packaging fall on the floor and get broken.

In general, microscopes should always be handled carefully because they are sensitive precision instruments. When using or transporting the microscope it is particularly important to avoid abrupt movements, as this may damage the optical components.

You should also avoid getting dirt or finger prints on the lens surface, because in most cases this will reduce image clarity.

To maintain the performance of the microscope, it must never be disassembled. So components such as lenses and other optical elements should be left as they were before use. Also the electrical parts on the rear and base of the device must not be tampered with, as in this area there is an additional risk of triggering an electric shock.

1.2 Notes on the electrical system

Before connecting to a mains power supply, you must make sure that you are using the correct input voltage. The information to select the correct mains cable is located on the device, on the rear of the product directly above the connection socket. You must comply with this information. If you do not comply with these specifications, then fires or other damage to the device could occur.

The main switch must also be switched off before the mains cable is connected. In this way you will avoid triggering an electric shock.

If you are using an extension cable, then the mains cable you use must be earthed.

When carrying out any procedures whereby you come into contact with the electrical system of the device, such as, for example, changing the bulb or fuse, only carry out these procedures when the power is disconnected.

1.3 Storage

You should ensure that the device is not exposed to direct sunlight, temperatures which are too high or too low, vibrations, dust or a high level of humidity.

The ideal temperature range is between 0 and 40°C and a relative humidity of 85% should not be exceeded.

The device should always be located on a rigid, smooth, horizontal surface.

When the microscope is not being used, you should cover it with the enclosed dust protective cover. When doing this, the power supply is stopped by switching off at the main switch and unplugging the mains cable. If the eyepieces are being stored separately, the protective caps must be fitted to the tube connectors. In most cases, if dust and dirt gets inside the optical unit of a microscope this can cause irreversible errors or damage.

The best way to store accessories which consist of optical elements, such as, for example, eyepieces and objectives, is in a dry box with desiccant.

1.4 Maintenance and cleaning

In any event, the device must be kept clean and dusted regularly.

If any moisture should occur, before you wipe down the device you must ensure that the mains power is switched off.

When glass components become dirty, the best way to clean them is to wipe them gently with a lint-free cloth.

To wipe oil stains or finger prints off the lens surface, moisten the lint free cloth with a mixture of ether and alcohol (70 / 30 ratio) and use this to clean the lens.

You must be careful when handling ether and alcohol, as these are highly flammable substances. You must therefore keep it away from naked flames and electrical devices which can be switched on and off, and only use it in well-ventilated rooms.

However organic solutions of this type should not be used to clean other components of the device. This could lead to damage to the paint finish. To do this, it is sufficient to use a neutral cleaning product.


You could also use the following cleaning products to clean the optical components:

- Special cleaner for optical lenses
- Special optical cleaning cloths
- Bellows
- Brush


When handled correctly and checked regularly, the microscope should give many years of efficient service.

Should repairs still be necessary, please contact your KERN dealer or our Technical Department.



2 Nomenclature

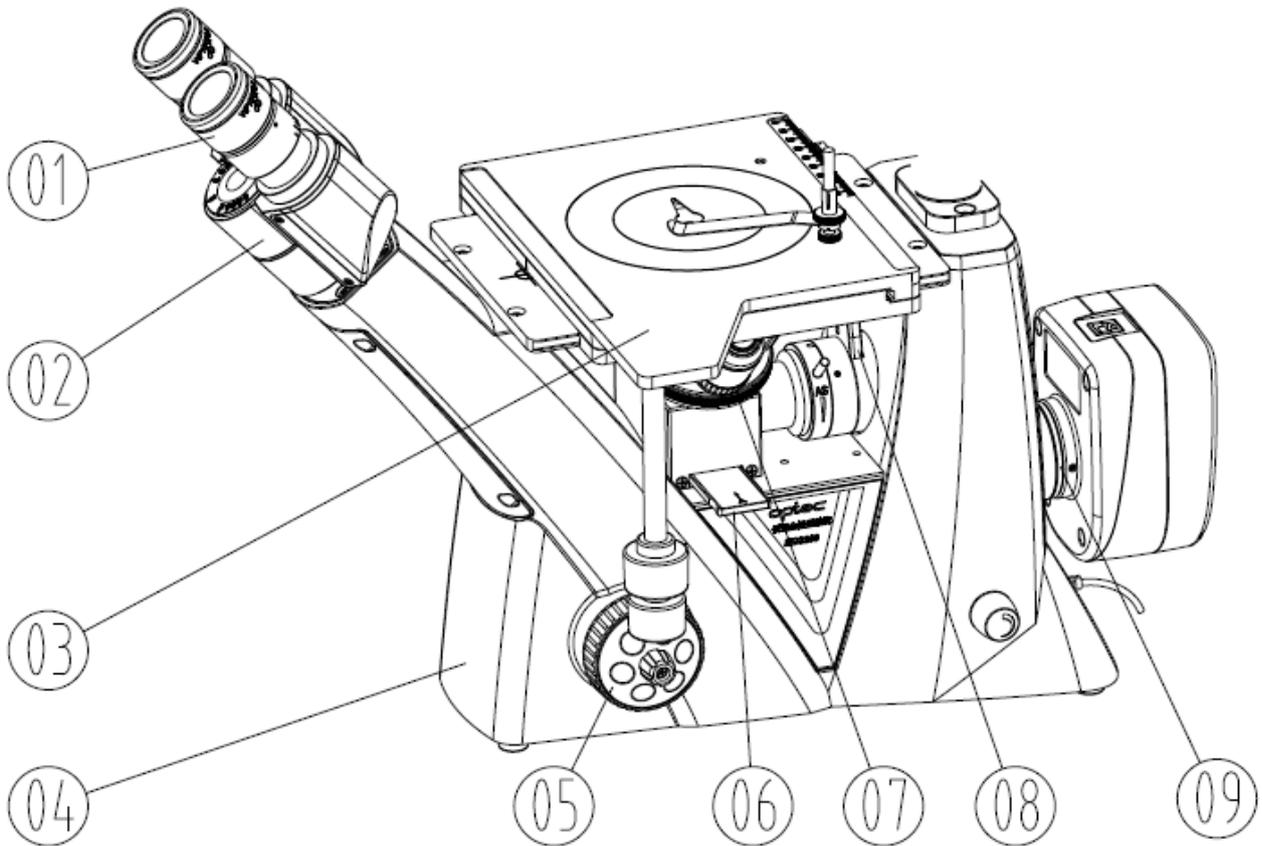

- ① Eyepiece
- ② Butterfly Siedentopf tube
- ③ Mechanical stage
- ④ Main body
- ⑤ Coarse & fine focusing knob
- ⑥ Analyser
- ⑦ Nosepiece
- ⑧ Polariser
- ⑨ 0.5X C-mount adapter for digital camera

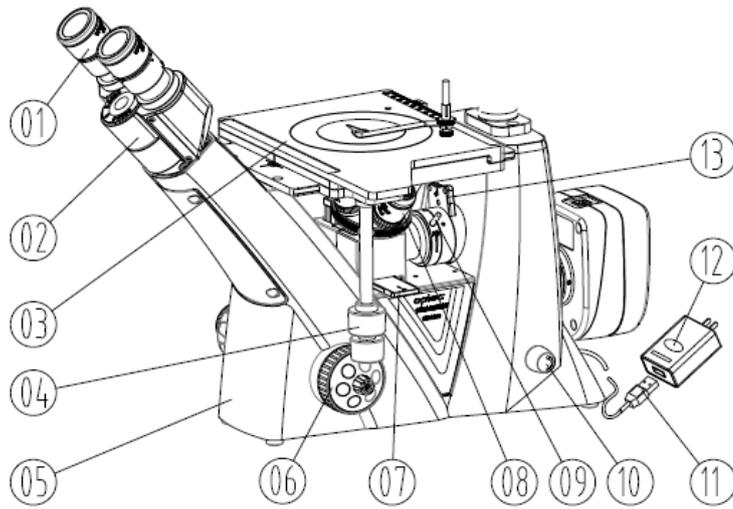

- | | |
|--------------------------------------|---|
| 1) Eyepiece | 12) Power supply adapter |
| 2) Butterfly Siedentopf tube | 13) Polariser |
| 3) Mechanical stage | 16) Microscope camera |
| 4) Stage adjusting hand wheel | 17) Locking screw for camera |
| 5) Main body | 18) Illumination unit |
| 6) Right coarse & fine focusing knob | 19) Left coarse & fine focusing knob |
| 7) Analyser | 20) Ø110 Sample holder |
| 8) Objective | 21) Sample holder Clip |
| 9) Aperture diaphragm lever | 22) DC Input Socket |
| 10) Dimmer knob | 23) 0.5X C-mount adapter for digital camera |
| 11) USB power line | |

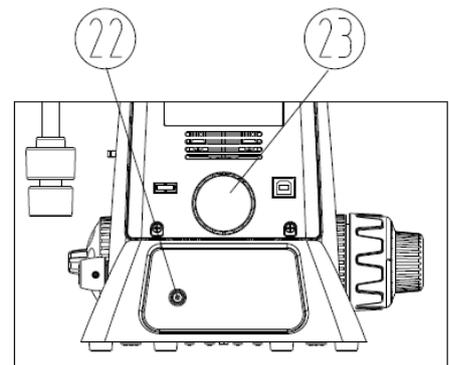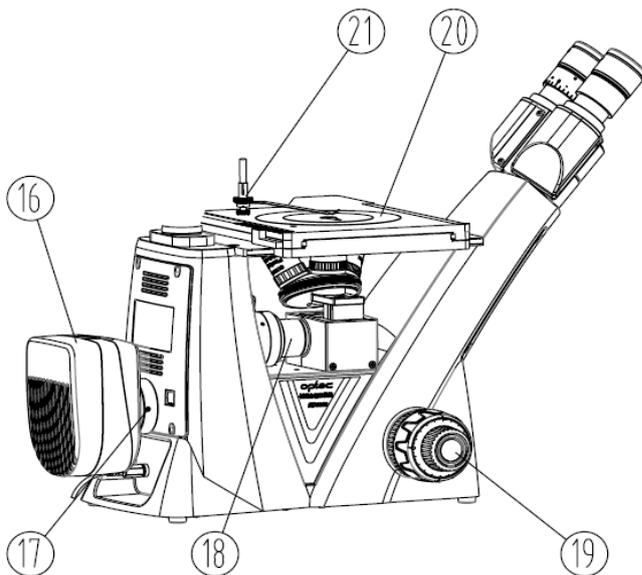

3 Technical data / Features

Model	Standard configuration				
	Tube	Eyepiece	Objective quality	Objectives	Illumination
KERN					
OLM 170	Trinocular	HWF 10×/∅ 20 mm	Infinity Plan	LWD5×/LWD10×/ LWD20×/LWD50×	5 W LED (incident)

Product dimension: 240x330x470 mm

Packing dimensions: 500x420x300 mm

Net weight: 7 kg

Gross weight: 9 kg

Input voltage: AC 100-240V, 50-60Hz


Output voltage: DC 5V, 1A

Model outfit		Model KERN	Order number
		OLM 170	
Eyepieces (23,2 mm)	HWF 10×/∅ 20 mm (adjustable)	✓	OBB-A1404
	WF 10×/∅ 20 mm (reticule 0,1 mm) (adjustable)	✓	OBB-A1532
Infinity Plan achromatic objectives for long working distance	5×/0,13 W.D. 16,04 mm	✓	OBB-A1525
	10×/0,25 W.D. 18,48 mm	✓	OBB-A1526
	20×/0,40 W.D. 8,35 mm	✓	OBB-A1527
	50×/0,70 (spring-loaded) W.D. 1,95 mm	✓	OBB-A1528
	80×/0,80 (spring-loaded) W.D. 0,85 mm	○	OBB-A1530
	100×/0,85 (dry) W.D. 3,00 mm	○	OBB-A1623
Trinocular tube	<ul style="list-style-type: none"> · Butterfly 45° inclined · Interpupillary distance 48-76 mm · Light distribution 20:80 · Diopter adjustment: One-sided 	✓	
Mechanical stage	<ul style="list-style-type: none"> · Stage size B×T 155×180 mm · Travel 75×40 mm · Coaxial coarse and fine focusing knobs 	✓	
Illumination	5 W LED spare bulb (incident)	✓	OBB-A1589
Reflected illumination unit	Polarising unit (Incl. analyser, polariser and colour filter slide)	✓	
Colour filters for transmitted illumination	Grey	✓	OBB-A1513
C-Mount	0,5× (built-in)	✓	

✓ = Included with delivery

○ = Option


4 Assembly

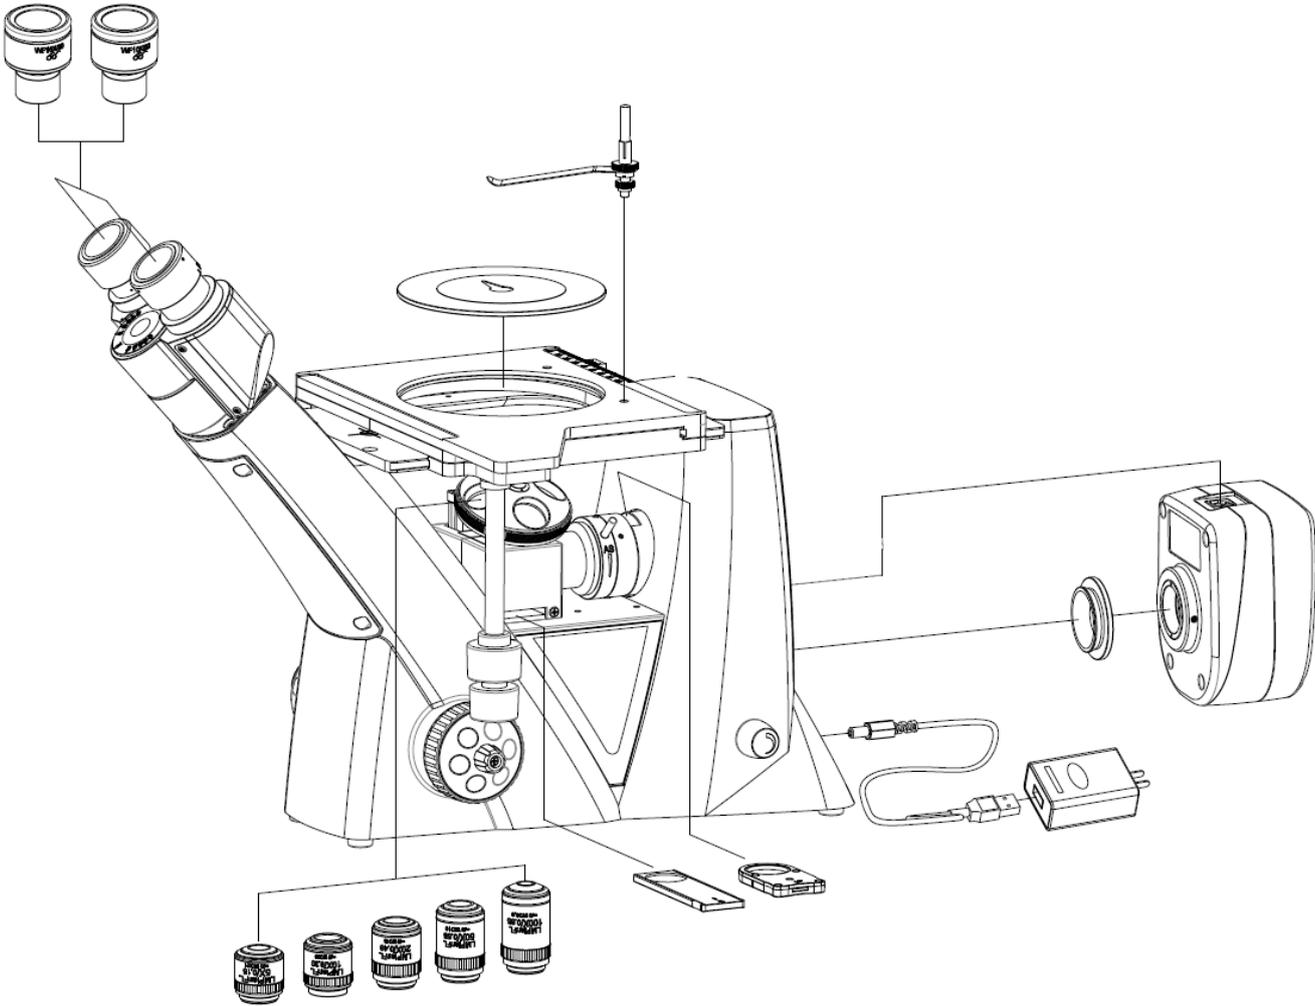


4.1 Reflected light unit

The reflected light unit consists of a light source (LED) located in the microscope housing and a polarisation unit.



For operation, the USB power cable [2] including the power supply adapter [1] must be connected to the power socket [3] on the rear of the microscope.

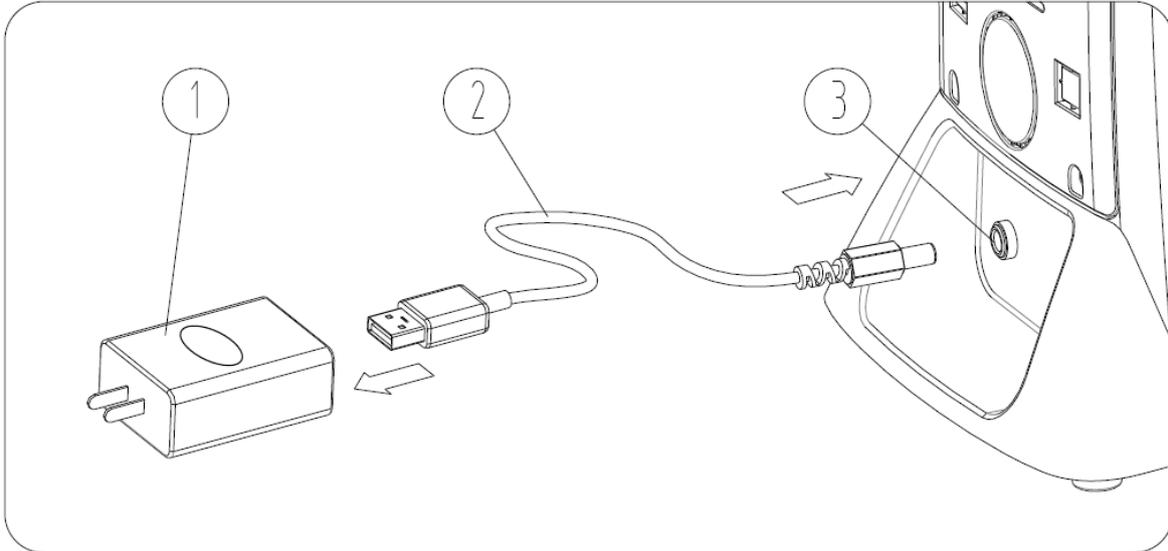

The aperture diaphragm [1] and a gray filter [2], which must also be inserted in the beam path, are used to modify the light in brightfield mode.

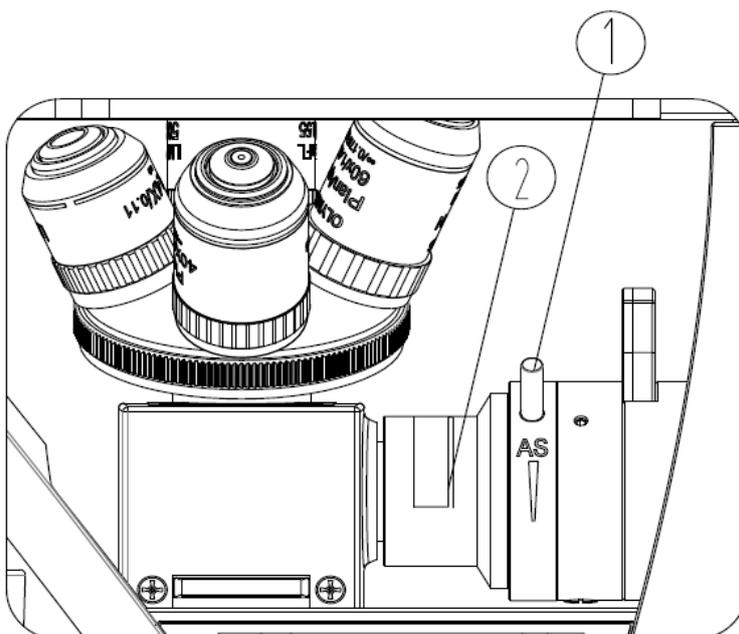

For the application of the polarization method, an analyser slide [3] and a polariser slide [1+2] are included in the scope of delivery, which must also be placed in the appropriate slots.

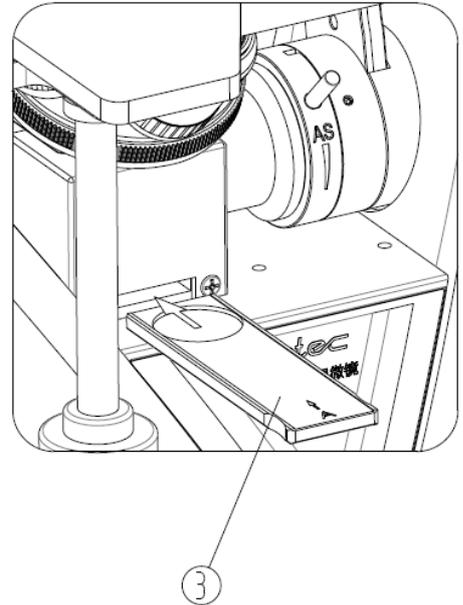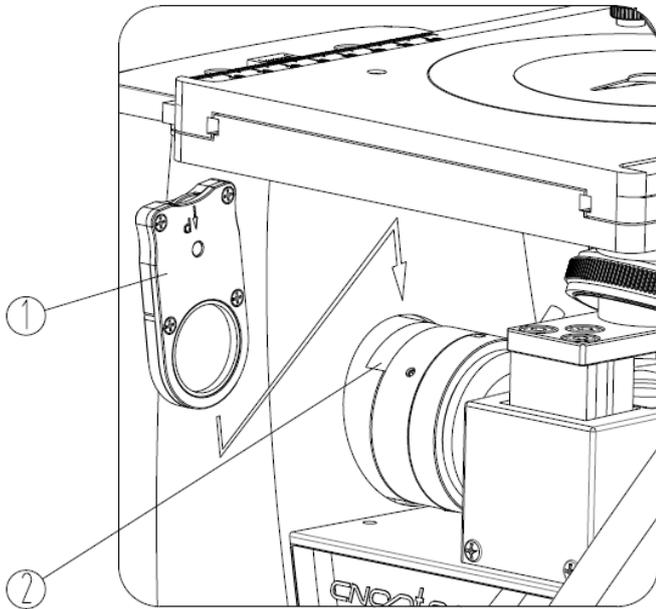

See also page 7:


Analyser slide / has the name "A" (7)

Polariser slide / has the name "P" (13)

4.2 Objectives


The nosepiece must be in its lowest position so that the objectives can be screwed into it. You can then pass the objectives through the opening of the specimen stage and screw them into the nosepiece, so that when you turn the nosepiece in a clockwise direction, the objective with the next strongest magnification appears. You must make sure that you do not touch the lenses with your bare fingers and that no dust enters the apertures.

To the screw locations which are not filled with an objective, you must attach the protective cap.

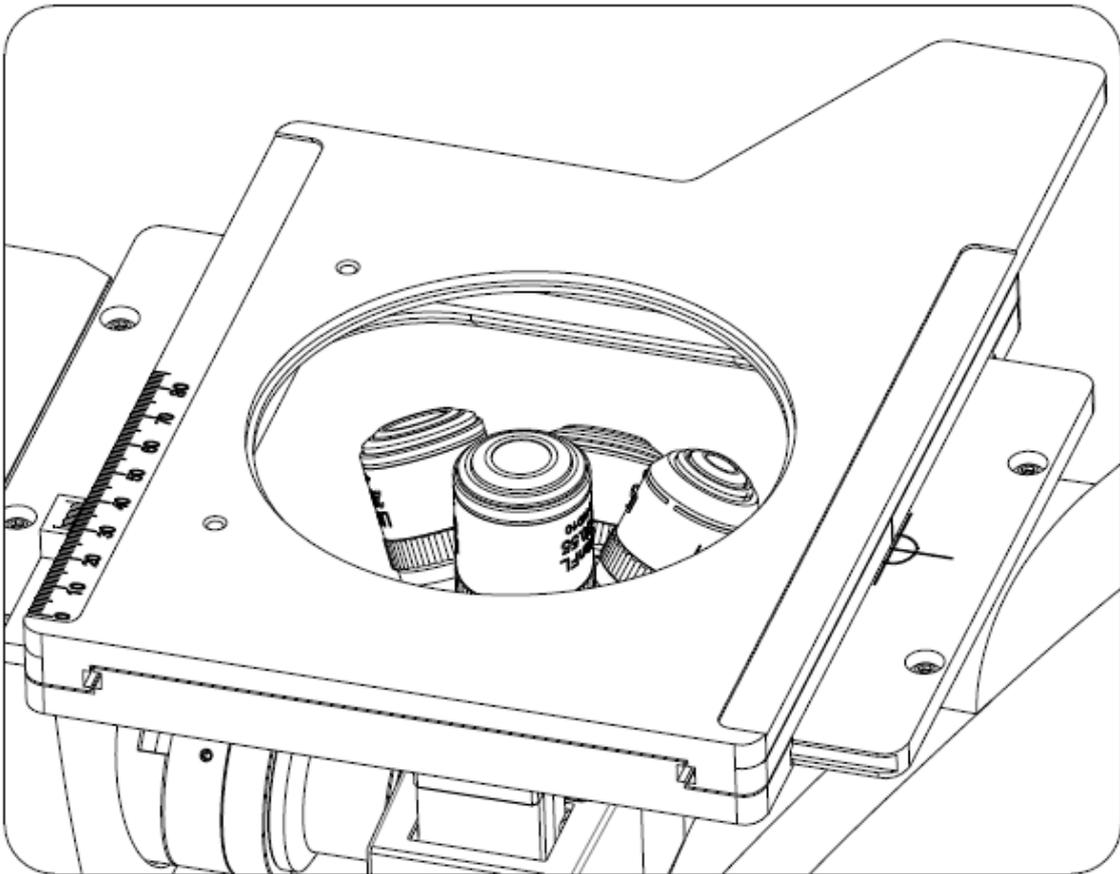

4.3 Eyepieces


You must always use eyepieces with the same magnification for both eyes. These are simply placed onto the tube connectors, once you have first removed the plastic protective caps. You should always make sure that you do not touch the lenses with your bare fingers and that no dust enters the apertures.

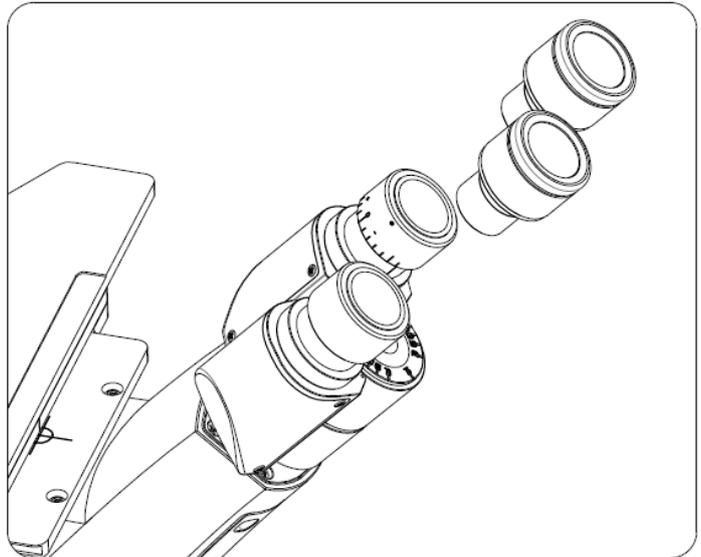

4.4 Specimen stage

The supplied stage plate [1] needs to be fitted to the opening of the specimen stage, in order to get a support area for relatively small observation objects and to protect the objectives which are located underneath.

Furthermore, you can attach an object holder clip [2] to one of the threads on the stage surface.

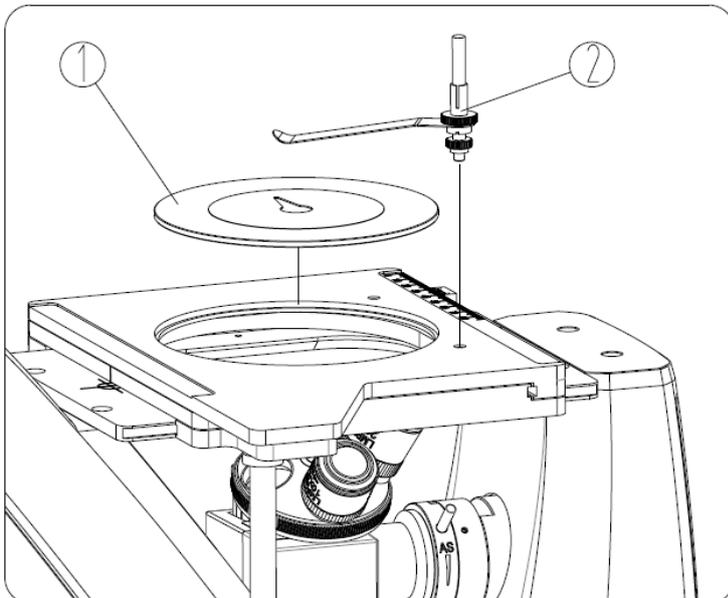

For the connection of a camera, please see Chapter 7 Use of optional accessories.



5 Operation

5.1 Getting started

The very first thing to do is to establish the power connection by means of the mains plug. Now the illumination can be switched on via the main switch (dimmer). The light intensity control (dimmer) should first be set to a low level so that the eyes are not immediately exposed to too much light when looking into the eyepieces for the first time.

The next step is to place an object on the specimen stage [1]. The object can be fixed on the stage using the object holder [2].


To move the spot of the object to be observed into the beam path, the dials on the right side of the stage must be operated accordingly (see *figure on the right [3]*). The marks for setting the stage center on the side of the object stage serve as orientation points (see *figure on the left [3]*).

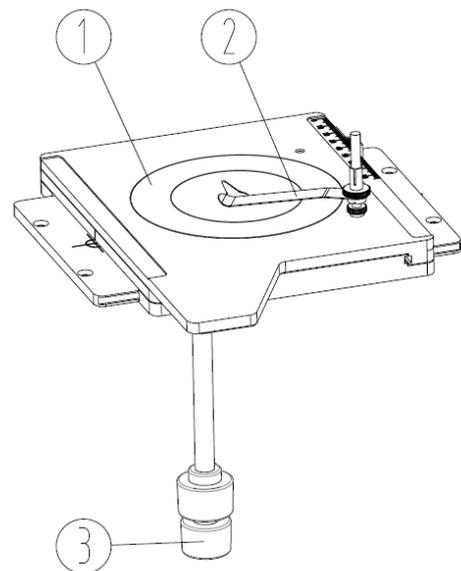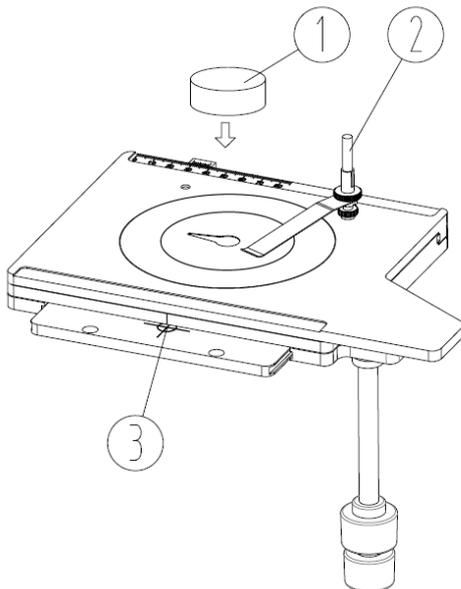

5.2 (Pre-) focussing

When you are observing an object, you must have the correct distance to the objective to achieve a sharp image.

In order to find this distance at the beginning (without other default settings of the microscope) place the objective with the lowest magnification in the beam path, look through the right eyepiece with the right eye and turn it slowly using the coarse adjustment knob.

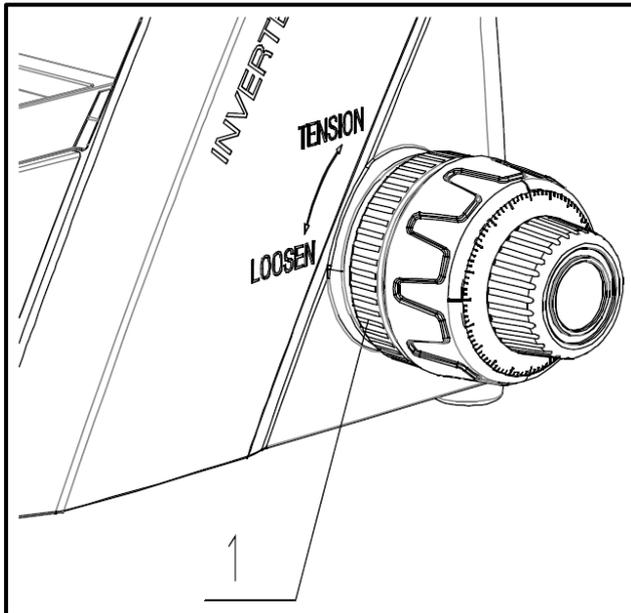

The simplest way of doing this would be to first raise the nosepiece (using the coarse adjustment knob) to the top position and then lower it slowly. As soon as an image is recognizable (no matter how sharp), then you should only adjust the focus using the fine adjustment knob.

Adjusting the torque of the coarse and fine adjustment knob

Next to the left adjustment wheel for the coarse and fine adjustment knob there is a ring (see illustration [1]) which you can use to alter the torque of these wheels. Turning it in a clockwise direction reduces the torque and turning it in an anti-clockwise direction increases it.

On one hand, this function can help to make it easier to adjust the focus and on the other hand it can prevent the nosepiece from slipping down unintentionally.


Important:

In order to avoid damaging to the focussing system, the left and right adjustment wheels for the coarse and fine adjustment knob must never be rotated at the same time in opposite directions.

5.3 Adjusting the interpupillary distance

With binocular viewing, the interpupillary distance must be adjusted accurately for each user, in order to achieve a clear image of the object.

While you are looking through the eyepieces, use your hands to hold the righthand and lefthand tube housing firmly. By pulling them apart or pushing them together, you can either increase or reduce the interpupillary distance (*see illustration*). As soon as the field of views of the lefthand and righthand eyepieces completely overlap each other, i.e. they combine to form a circular image, then the interpupillary distance is set correctly.

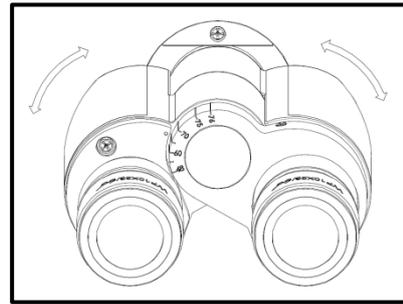


5.4 Diopter adjustment

The eye strengths of each eye of the microscope user can often be slightly different, which in daily life has no consequences. But when using a microscope this can cause problems in achieving precise focusing.

You can use a mechanism on both tube connectors (diopter adjustment rings) to compensate for this as follows.

1. Look through the right eyepiece with the right eye and bring the object into focus by using the coarse and fine adjustment knob.
2. Then look through the left eyepiece with the left eye and use the diopter adjustment ring to focus the image.
To do this, you just need to turn the ring in both directions (*see illustration*), to find out where the image is at its most focussed.

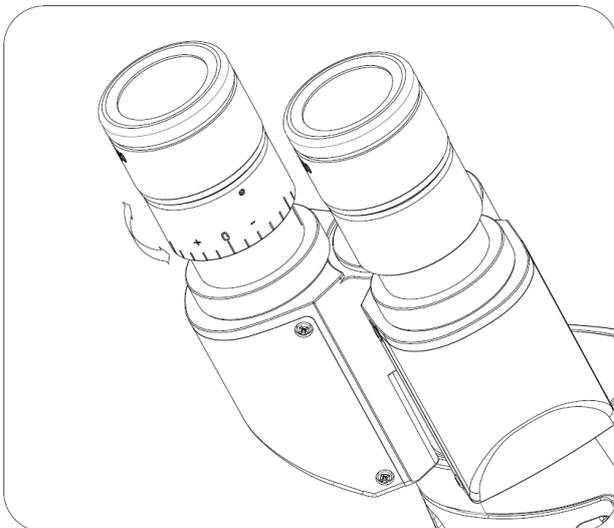

5.5 Adjusting the magnification

After pre-focusing has been carried out using the objective with the lowest magnification (*see section 5.2*) you can then adjust the overall magnification using the nosepiece, as necessary. By turning the nosepiece you can bring any one of the four other objectives into the beam path.

When adjusting the nosepiece, you must take the following points into account:

- The required objective must be properly locked in place at all times.
- The nosepiece should not be rotated by holding individual objectives. You should use the black ring below the objectives.
- When rotating the nosepiece you must always make sure that the objective which is about to be positioned in the beam path does not touch the stage plate. This can lead to significant damage to the objective lens.
We recommend that you always check from the side to make sure that there is sufficient leeway. If this should not be the case, the nosepiece must be lowered accordingly.

If you have focussed the object to be observed for a specific magnification, then if you select the objective with the next greatest magnification, the object will be slightly out of focus. Use the fine adjustment knob to make a slight adjustment and restore the focus.

5.6 Using eye cups

The eye cups supplied with the microscope can basically be used at all times, as they screen out intrusive light, which is reflected from light sources from the environment onto the eyepiece, and the result is better image quality.

But primarily, if eyepieces with a high eye point (particularly suitable for those who wear glasses) are used, then it may also be useful for users who don't wear glasses, to fit the eye cups to the eyepieces.

These special eyepieces are also called High Eye Point eyepieces. They can be identified by the glasses symbol on the side. They are also marked in the item description by an additional "H" (example: HSWF 10x Ø 23 mm).

When fitting the eye cups, make sure that the diopter setting is not moved. We would therefore advise that you hold the diopter compensation ring on an eyepiece with one hand while you fit the eye cup with the other.

Before using the microscope, users who wear glasses must remove the eye cups, which you may find on High Eye Point eyepieces.

As the eye cups are made of rubber, you must be aware that when you are using them, they can become slightly dirty through grease residues. In order to maintain hygiene, we would therefore recommend that you clean the eye cups regularly (e.g. with a damp cloth).



Eye cups



High Eye Point eyepiece
(identified by the glasses symbol)

5.7 Adjusting the illumination

To make sure that perfect image results are achieved during microscopic observation, it is important that the direction of light of the microscope is optimised. The following components of the reflected light unit can be adjusted according to the application requirements.

Aperture diaphragm

(See page 11)

The aperture diaphragm allows the optimum compromise between contrast and resolution to be set for the microscopic image.

Opening and closing of this aperture is performed via the lever located on the top of the incident light unit.

Colour filter

(See page 11)

The colour filter slider contains a permanently integrated gray filter. If required, this must be placed in the corresponding slot on the illumination unit.

Polarising unit (Analyser / Polariser)

(See page 12)

The OLM 170 series provide the possibility to apply the contrasting method of polarised light. For this purpose the analyser and polariser (both of them are included with the scope of delivery) are used.

In order to bring the analyser into the beam path you must attach the analyser slide to the slot, located underneath the nosepiece. Both the slide and the slot have the name "A".

Next to the field and aperture diaphragm the slot for the polariser is located. Both the slide and the slot have the name "P". The integrated wheel on the polariser slide is facing out after attaching it to the slot. With the wheel you can control the required alignment of the polariser.

6 Changing the bulb

If a defect occurs in the lighting unit or other electrical components, the Technical Service department of Kern & Sohn GmbH must be contacted for repair.

7 Using optional accessories


7.1 Camera connection

Due to an additional beam exit at the rear of the microscope it is possible to connect microscope cameras to the device, in order to digitally record images or sequences of images of an object being observed.

After removing the plastic cover on the camera adapter (C-mount 0.5x), which is already located on the camera connection on the back of the microscope, a camera that has a C-mount thread can now be screwed onto the adapter.

The following steps are recommended for optimal mounting:

1. Loosen the locking screw [4] on the camera connection [3] and remove the C-mount adapter [2].
2. Screw the C-mount adapter [2] onto the microscope camera [1].
3. Connect the microscope camera [1] together with the C-mount adapter [2] to the camera connection [3] and tighten the locking screw [4] again.

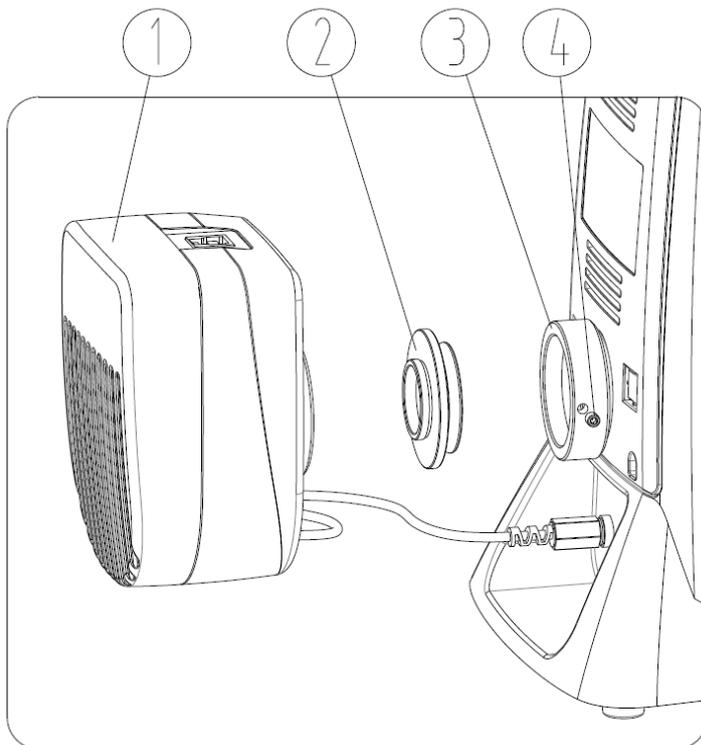

The light from the microscope illumination is permanently provided in the beam path for both the camera and the eyepieces, so that analog and digital observation is always possible simultaneously.

8 Trouble shooting

Problem	Possible causes
The bulb does not light	The mains plug is not correctly plugged in
	There is no power at the socket
	Defective bulb
	Defective power supply adapter
The bulb blows immediately	The specified bulb or fuse has not been used
The field of view is dark	The aperture diaphragm and/or field diaphragm are not opened wide enough
	The condenser is not correctly centred
You cannot adjust the brightness	The brightness control has been set incorrectly
	The condenser has not been correctly centred
The field of view is dark or is not correctly illuminated	The objective is not positioned correctly on the beam path
	The nosepiece is not correctly fitted
	An objective is being used which doesn't match the lighting area of the condenser
	The condenser has not been correctly centred
The field of view of one eye does not match that of the other eye	The interpupillary distance is not correctly adjusted
	Dioptre setting has not been carried out correctly
	Different eyepieces are used for the righthand and lefthand side
	The eyes are not used to using a microscope

Problem	Possible causes
Blurred details Bad image Bad contrast Vignetted field of view	The aperture diaphragm is not opened wide enough
	The objective does not belong to this microscope
	The front lens of the objective is dirty
	The condenser is not correctly centred
	Dirt / dust on the objective
Dirt or dust in the field of view	Dirt / dust on the eyepieces
	Dirt / dust on the object
One side of the image is blurred	The stage was not correctly fitted
	The objective is not positioned correctly on the beam path
	The nosepiece is not correctly fitted
The image flickers	The nosepiece is not correctly fitted
	The objective is not positioned correctly on the beam path
	The condenser has not been correctly centred
The coarse adjustment knob is difficult to turn	The rotational resistance brake is too tight
	The angle table is blocked by a solid body
When you move the table, the image becomes blurred	The stage was not correctly fitted

9 Service

If, after studying the user manual, you still have questions about commissioning or using the microscope, or if unforeseen problems should arise, please get in touch with your dealer. The device may only be opened by trained service engineers who have been authorised by KERN.

10 Disposal

The packaging is made of environmentally-friendly materials, which you can dispose of at your local recycling centre. Disposal of the storage box and device must be carried out by the operator in accordance with all national or regional laws in force in the location of use.

11 Further information

The illustrations may differ slightly from the product.

The descriptions and illustrations in this user manual are subject to change without notice. Further developments on the device may lead to these changes.



All language versions contain a non-binding translation.
The original German document is the binding version.

